


Appearance

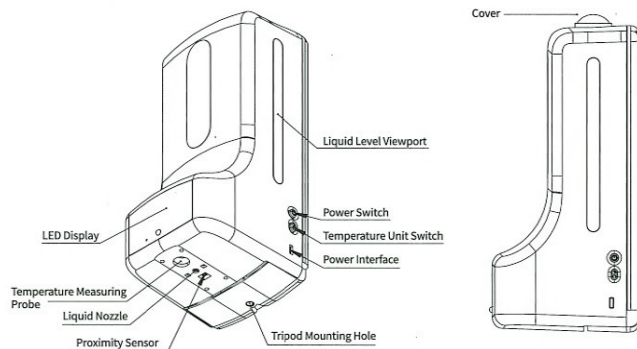

Specification

1. Accuracy: $\pm 0.2^{\circ}\text{C}$ (34~45 $^{\circ}\text{C}$ ZZ, put it in the operating environment for 30 minutes before use)
2. Alarm type: flashing + bleeping "DIDIDI"
3. Measuring distance: 5cm~10cm
4. LED display: Number
5. Interface: USB Type-C Port
6. Bottle Capacity: 1000ml
7. Mounting Type: Wall-hanging, Tripod-fixed
8. Working Temperature: 10 $^{\circ}\text{C}$ ~40 $^{\circ}\text{C}$ (15 $^{\circ}\text{C}$ ~35 $^{\circ}\text{C}$ Recommended)
9. Measuring range: 0~50 $^{\circ}\text{C}$
10. Response time: 500ms
11. Standby time: 5s for non-working, dynamic loop with white light
12. Input: DC 5V 1500MA
13. Dimension: 119*133*280mm
14. Liquid type: hand sanitizer

Conditions

1. Standby: the white dot on the bottom of right corner flashing by turns. (Fig. 1)



(Fig.1)

2. Normal temperature: displays current temperature and green light flashes once on the display. (Fig. 2)




(Fig. 2)

3. Abnormal temperature: displays current temperature and red light flashes on the display. (Fig. 3)



(Fig. 3)

4. Out of measuring range: "Lo": Ultra-low temperature alarm. (Fig. 4); "Hi": Ultra-high temperature alarm. (Fig. 5)




(Fig. 4)



(Fig. 5)


Instructions

1. Temperature measuring and hand washing: Put your hand on the bottom until you hear a "Di" sound, then the LED screen will display the temperature and hand sanitizer squeezed out. (Fig. 6)




(Fig. 6)


2. Temperature unit switch: Press C/F button on the right side of the device. (Fig. 7), the LED screen will display C or F, C:centigrade, F: Fahrenheit. (Fig. 8 and Fig. 9)



(Fig. 7)



(Fig. 8)



(Fig. 9)


Mounting

- (1) Tripod mounting: There is screw connection on the bottom which can be connected with tripod. (Fig. 10)




(Fig. 10)

- (2) Wall-hanging: There are two hanging holes on the back side can be fixed with nail. (Fig. 11)



(Fig. 11)

(3)Power On/Off: Press the switch button on the right side of the device. (Fig.12)

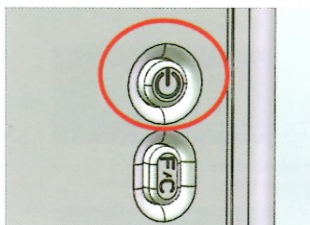


(Fig. 12)

Warnings

1. Do not pour hand sanitizer into Temperature Measuring Probe and Proximity Sensor.
2. Make sure that it is standing upright after filling in hand sanitizer.

Intelligent Sensor Soap Dispenser

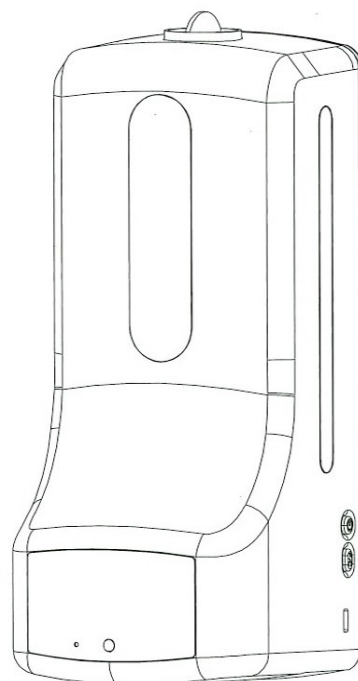

CE FCC RoHS
Made in China



K9